

## Main Auger Sensors



## REPLACEMENT SHEET

### Absorption Gamma on Main Auger

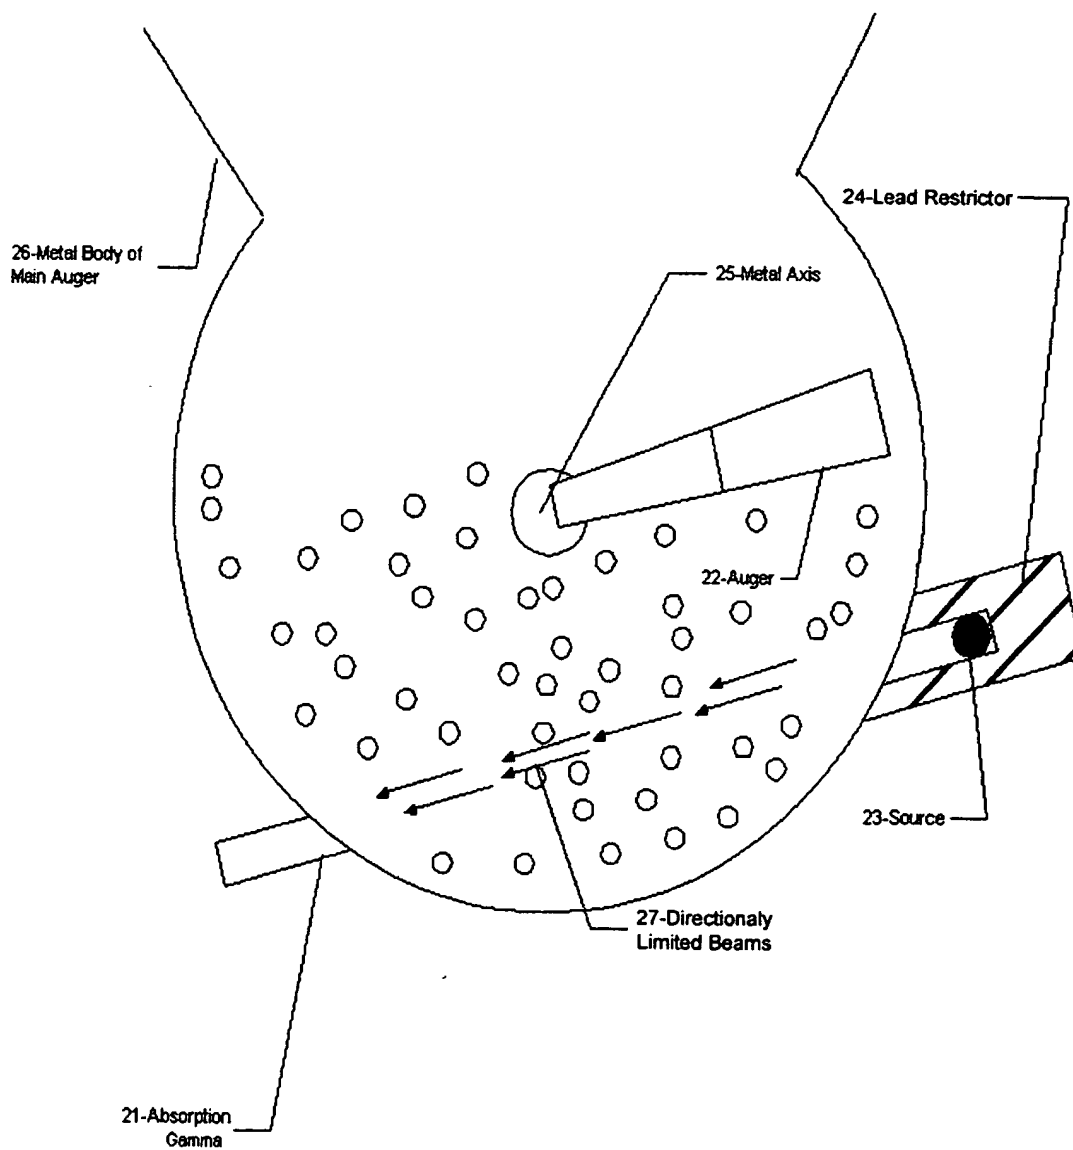


Fig. 2

## REPLACEMENT SHEET

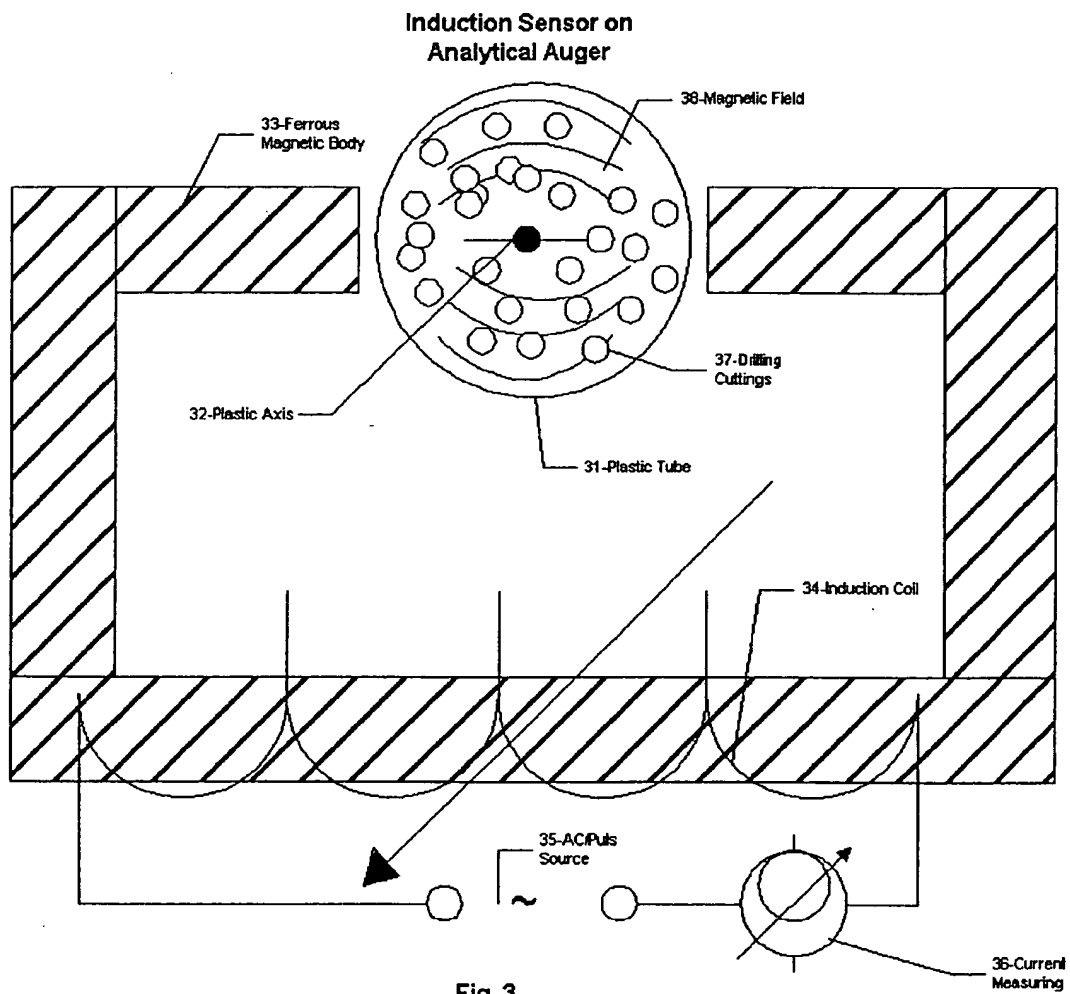


Fig. 3.

## REPLACEMENT SHEET

### Sonic Sensor on Analytical Auger

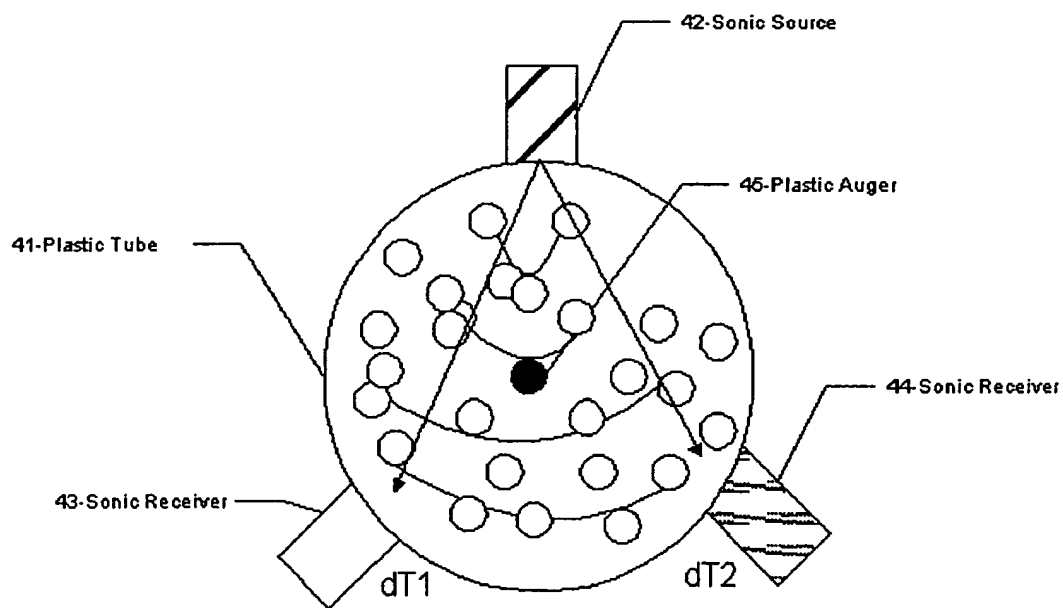


Fig. 4.

## REPLACEMENT SHEET

### Fluorescence Sensor in Analytical Tube

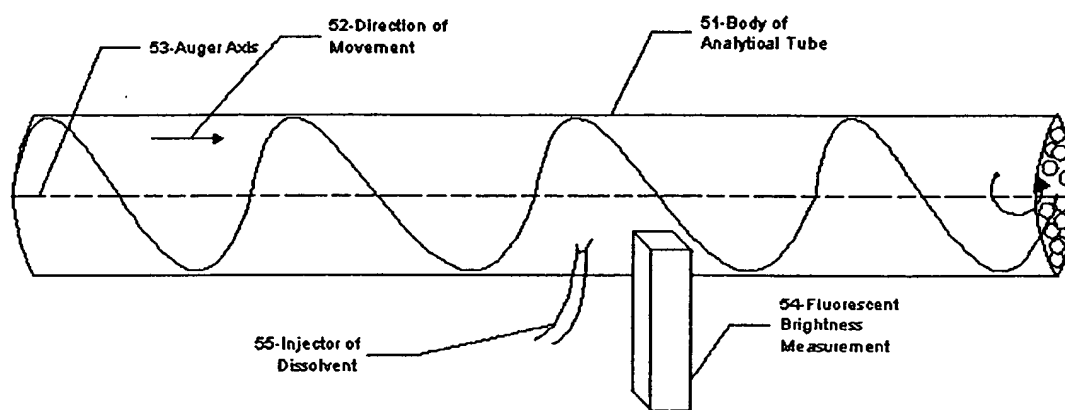


Fig. 6.

## REPLACEMENT SHEET

### Directional Restriction of Gamma Source

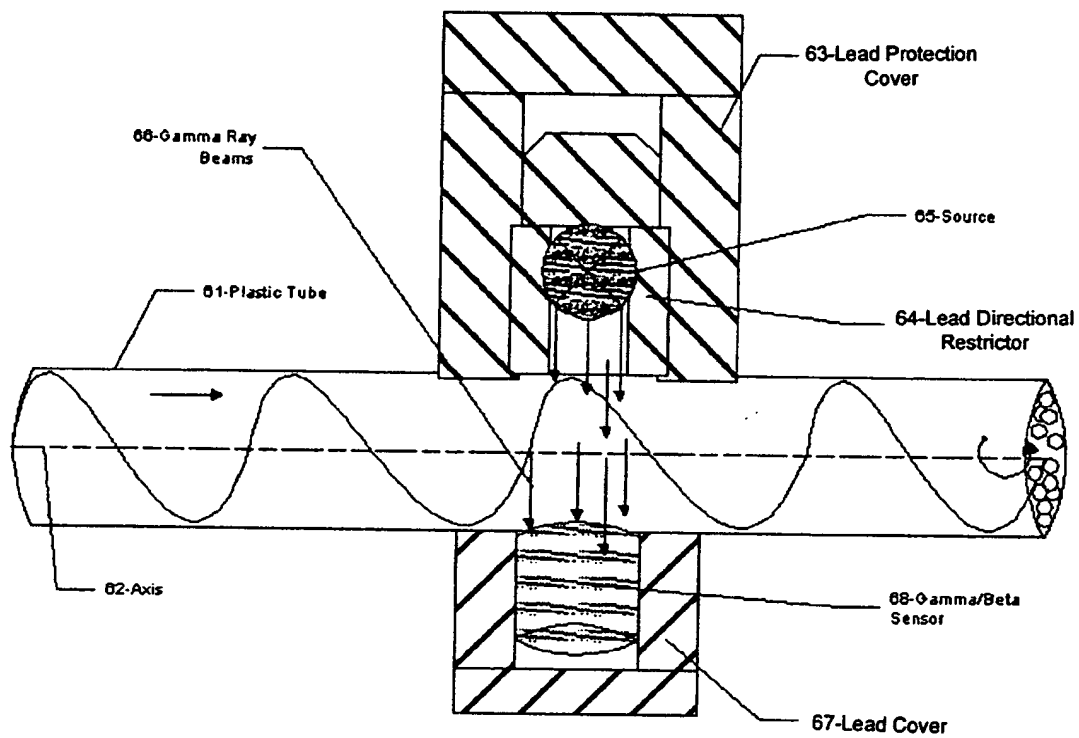


Fig. 6.

BEST AVAILABLE COPY